



Shore Sales Model 920 Moisture Meter

TESTING HOT GRAIN WITH THE MODEL 920 MOISTURE METER

To achieve accurate moisture results, moisture meters must be able to sense the sample temperature and apply a temperature correction. The model 920's sample temperature sensor will provide very accurate compensation for grain temperatures up to 110 °F and will also provide reasonably good results up to 160 °F, if samples are of uniform temperature. When the model 920 senses that the sample temperature is above 110 degrees, the moisture display will contain the word "Hot" to alert the user to potential problems with the results, as outlined below. When "Hot" is displayed, we suggest that you test the sample 3 times and take an average of the results.

There are several problems that can be encountered when testing hot grain from a dryer.

- The sample may not be a uniform temperature throughout (Some kernels hotter than others).
- The temperature of the individual kernels will not be the same throughout the kernel.
- The temperature of the grain will be changing rapidly.
- The kernels are not all the same moisture level, so the sample may not be representative.
- The hot grain is still expelling moisture. Since there is now no air movement over the grain, a film of water will form on the exterior of the grain kernels. Surface moisture can cause moisture meters to give erroneous results. (If many kernels stick to the sides and bottom of the grain cell when you dump the grain out, then you probably have excessive surface moisture.)

Since the amount of temperature compensation required is related to the moisture level of the grain, high temperatures in higher moisture grain will cause more problems than in dry grain below 16%. (We are compensating mainly for the temperature of the water in the grain) Typically, hot grain from the dryer that tests 18 to 25 % will test from 0.5% to 1.5% wetter if it is put in a sealed container and allowed to stabilize for an hour or two. Grain below 18% will show a smaller moisture gain.

Two things happen when the hot grain is allowed to stabilize in a sealed container.

- (1) The temperature throughout the sample and individual kernels becomes uniform.
- (2) Moisture distribution levels throughout the sample and kernels become more uniform.

These are the types of grain conditions that all moisture meter calibrations are based upon and therefor, these conditions result in the most accurate test results. This also more closely duplicates the conditions achieved by "steeping" the grain before binning.

If time allows, it is always best to let the hot grain sample cool and stabilize for an hour or two before testing. At the very minimum, the sample should be allowed to stabilize for at least 5 minutes, then mixed well before removing a portion for testing. This sample should be tested 3 times and averaged. If it is not possible to completely stabilize the sample, then a manual correction to the moisture result may be required to accurately determine the "real final moisture" of the sample. The amount of correction needed may have to be determined by experimentation.

If you have questions, contact Shore Sales Co. at (800) 837-0863 or (217) 892-2544

Rev July 2010

THE SHORE MODEL 920 MOISTURE METER

Introduction: The model 920 is a precision moisture meter that provides quick and accurate moisture results. The results are displayed automatically without the need for moisture or temperature conversion tables. When used within the specified operating limits, the model 920 will produce moisture results that are as accurate as commercial moisture meters costing thousands of dollars more. The model 920 has been designed to meet or exceed NIST handbook 44 specifications for grain moisture meter accuracy. These are the same accuracy specifications that commercial "Legal for Trade" moisture meters must meet.¹ Some of the unique features that allow the model 920 to achieve this level of accuracy are listed below.

Proven design: The grain test cell and sample dump cell were designed to replicate the cells found in the moisture meter that was used for more than 30 years to perform official grain inspections in the U.S. The calibrations for the model 920 were derived from the calibrations for that meter and have over 30 years of calibration data behind them.

Representative samples: Like commercial moisture meters, the model 920 uses a large (typically 250 grams) test sample to assure that the sample is representative of the entire load. Most other transportable moisture meters use a much smaller sample; some use a sample as small as 20 grams. Studies have shown that the moisture level of corn kernels can vary by a couple of percent from one end of the ear to the other and vary by several percent from different areas of a field. Small test samples may not contain enough kernels to be representative.

Moisture as a percentage by weight: The model 920 uses a pre-weighed sample. Moisture content is determined as a percentage by weight. It is difficult to determine moisture content accurately without knowing the weight. Some moisture meters use unreliable internal spring mechanisms to try to determine the weight of the sample; others just guess or ignore sample weight altogether.

Consistent sample loading: The model 920 uses a proven grain dump cell design. The mechanical dump cell insures that the grain will flow evenly and at a consistent rate into the grain test cell. The density or degree of packing of the grain in the grain test cell will affect moisture results. The mechanical loading method provided by the dump cell insures that the grain will flow into the test cell in a consistent manner that will produce repeatable results. With some meters, the user just pours in the sample. It is very difficult to pour the grain evenly and at the same rate all the time, so repeatability and accuracy suffer.

Test weight compensation: The model 920's unique grain cell design also compensates for variations in test weight. Test weight is a function of the kernel density. High test weight grains are more dense while low test weight grains are less dense. Grain density will affect moisture results. Most moisture meters will give higher moisture results on high test weight grains and lower results on low test weight grain so some type of compensation must be made for test weight variations. Other moisture meters just ignore test weight, so their accuracy falls off when the test weight varies.

Temperature compensation: Grain calibrations are specified at some reference sample temperature. This reference temperature is usually 77 °F or 25 °C. When grain is warmer than the reference temperature; the moisture results will be higher than actual moisture. The results will be lower when the grain temperature is below the reference temperature. The temperature correction required for each grain varies and can range from about 0.05% per °F to 0.1% or more per °F. As you can see, a few degrees error in temperature measurement can cause a significant error in moisture results. Accurate temperature compensation becomes extremely important when the grain is very cold or very hot. The temperature correction for a sample of 21% moisture corn at 40 °F can be as much as 2.6%!

In addition, when the temperature of the grain is more than a few degrees above or below the ambient temperature of the meter, a greater amount of time is required to allow the temperature sensor to accurately sense the grain temperature. The model 920 uses a quick response, precision temperature sensor that will accurately measure sample temperature to within +/- 1 degree F. The model 920 uses an intelligent process to determine when it should allow more time to accurately sense the temperature. Samples close in temperature to the meter will test in only a few seconds, while extremely hot or cold samples will take up to 25 seconds to accurately measure the temperature. The model 920's temperature compensation rates among the best of any moisture meter on the market, including commercial grade meters.

Available calibrations: The standard model 920 includes calibrations for the most common grains. There are currently about 100 different calibrations for the model 920 that are available by special request. These calibrations include processed and unprocessed rice, edible beans & peas, coffee, peanuts, vegetable and grass seeds and many other commodities. Please contact Shore Sales Co. for a complete list of available calibrations.

A complete moisture testing package: The model 920 is available packaged in a sturdy protective carrying case along with a precision portable electronic scale for sample weighing. Both the model 920 and the scale can be powered by internal batteries, or by the included external AC adapters. Power options for the 920 include power adapters that plug in automobile cigarette lighter sockets.

The next few pages explain how to use the model 920 moisture meter to obtain quick and accurate moisture tests.

Notes: (1) Although the 920 meets NIST handbook 44 tolerances it may not be used in "Legal for Trade" applications in states that require NTEP certification for moisture meters.

SHORE MODEL 920 MOISTURE METER OPERATING INSTRUCTIONS

1. Turn on meter. The 920 will perform an internal self-test while displaying model, serial number and software version.
2. The 1st grain calibration will be displayed. Use UP or DOWN arrows to display other available grains.
3. When the desired grain is displayed, press TEST. The 920 will display "Wait" while it performs internal calibration for that grain.

While performing the internal calibration, the 920 will check to make sure that the grain cell does not already contain a sample. If this is the case, the operator will be prompted to "Empty the cell and press a key".

4. The display will then show the required sample size and prompt the operator to load and test the sample.
5. Weigh the required amount of the grain and put it into the top chamber of the dump cell.
6. Place the dump cell containing the sample onto the grain cell.
7. Press the dump cell knob to load the sample, then remove the dump cell and press TEST.

(When you remove the dump cell, flip it over and it will automatically reset and be ready for the next sample.)

The 920 will display "Wait" while the sample is being tested and then display the sample temperature, followed by the moisture. The 920 will delay from 3 to 25 seconds before displaying results. (The length of the delay is dependent on the grain temperature relative to the ambient temperature. The closer the grain temperature to ambient, the shorter the delay.)

8. Dump the sample out of the grain test cell and press TEST to perform another test on the same grain or select a different grain. (While the moisture results are being displayed, the UP or DOWN ARROW keys can be used to switch between temperature and moisture.)
9. If viewing the display in very dim light, pressing the button located towards the right rear corner of the console will turn on the display backlight brighten the display.

Special grain conditions:

1. When testing high moisture corn, the large sticky kernels will sometimes lodge between the cell center post cone and the cell tube. If this occurs, just flick them down into the cell before pressing the TEST key. The level of the grain in the test cell should be below the bottom of the white cone for an accurate test.
2. Like all moisture meters, the model 920 grain calibrations are based on good quality, clean grain samples. Quality factors such as moldy grain, excessive dirt or foreign materials may affect accuracy.

TESTING HOT GRAIN:

To achieve accurate moisture results, moisture meters must be able to sense the sample temperature and apply a temperature correction. The model 920 has a very accurate sample temperature sensor located in the test cell and will provide excellent compensation for grain temperatures up to 120 °F. The model 920 can provide reasonably good results up to 160 °F for samples that are of uniform temperature. When the model 920 senses that the sample temperature is above 120 degrees, the moisture display will contain the word "Hot" to alert the user to potential problems with the results, as outlined below. When "Hot" is displayed, we suggest that you test the sample 3 times and take an average of the results.

When testing grain samples above 120 °F that are from a grain dryer, results may require adjustment. There are several problems with testing hot grain from a dryer. One is that the sample may not be a uniform temperature throughout (Some kernels may be hotter than others). Another is that the temperature of the individual kernels will not be the same throughout the kernel. (The exterior of the kernel may be hotter than the interior). The latter condition where the kernels are hotter on the outside can result in the sensed temperature to be higher than it really is.

Here are some of the problems that can be encountered when testing hot grain from a dryer.

- The sample may not be a uniform temperature throughout (Some kernels hotter than others).
- The temperature of the individual kernels will not be the same throughout the kernel.
- The temperature of the grain will be changing rapidly.
- The hot grain is still expelling moisture. Since there is now no air movement over the grain, a film of water will form on the exterior of the grain kernels. Surface moisture can cause moisture meters to give erroneous results. (If many kernels stick to the sides and bottom of the grain cell when you dump the grain out, then you probably have excessive surface moisture.)

For best accuracy, the sample should be allowed to stabilize before testing. The best way to stabilize the sample is to spread it out on a screen that will allow air to circulate over, under and around the grain. After two or three minutes, the sample should be ready to test.

If a screen is not available, an alternate method is to pour the grain back & forth between two containers until it is stable.

If time allows, it is always best to let the hot grain sample cool and stabilize before testing. If this is not possible then a manual correction to the moisture result may be required to accurately determine the "real final moisture" of the sample. The amount of correction needed may have to be determined by experimentation.

MOISTURE TESTING ACCURACY:

When discussing the accuracy of moisture tests, we must first define a reference for comparison. There are two categories of references. These are the “Primary” and “Secondary” references.

The Primary reference standard is the air oven. In the air oven method, samples of grain to be tested are ground to a specific particle size, precisely weighed and then they are heated in the ovens at specified temperatures for specified periods. The samples are then re-weighed and the original moisture level computed by using the weight loss in drying. The procedures for performing air oven tests on various types of grain are specified in the USDA “Moisture Handbook”. The air oven test takes from one hour to more than 72 hours depending on the type of grain and moisture levels. Since the “Primary” method requires a laboratory, lots of specialized equipment and a lot of time, it is not suitable for everyday moisture testing.

The “Secondary” reference is usually a moisture meter that has been calibrated to closely match the air oven. This secondary standard is then used to verify the calibration of other moisture meters. The main problem that occurs with this secondary method, is that various manufacturers’ moisture meters, including the secondary standard, may react differently to new strains and hybrids, and differing grain quality. This is the reason that all moisture meter calibrations should be referenced to the primary standard air oven.

It must also be understood that hundreds and sometimes thousands of grain samples from several crop years are used to develop grain calibrations. The resulting calibrations are “averages” of all the samples tested and some samples that lie at the extremes of the averages may show a full percent or more of deviation from the “average”.

The Model 920 grain calibrations are referenced to the primary standard air oven and all accuracy specifications for the model 920 are in reference to the air oven results. Also bear in mind that as previously stated, grain calibrations are based upon averages of many samples and occasionally you may test a sample that deviates by a large amount from the average. The maximum accuracy tolerance specifications for the model 920 are the same as those specified in NIST handbook 44. These are maximum tolerances and the 920 typically will be within ½ of the maximum tolerance when compared to the standard air oven method.

Specifications for grain moisture meters used in “Legal For Trade” applications in the U.S. are published by the National Institute of Standards and Technology (NIST) in NIST handbook 44. The HB 44 tolerances for grain moisture meters are as follows.

Type of Grain or Seed	Tolerance	Minimum Tolerance
Corn, Oats, Rice, Sorghum, Sunflower	0.05 of the percent moisture content	0.8 percent in moisture content
All other cereal grains And oilseeds	0.04 of the percent moisture content	0.7 percent in moisture content

Error messages: The model 920 tests its internal circuits whenever the power is switched on. The tests and error messages are listed below.

POWER-ON TESTS: The following tests are performed when the 920 is first turned on.

Battery check: If the battery voltage becomes too low for reliable operation, the 920 will display "Batt Low". This message indicates that the battery should be replaced as soon as possible.

Grain cell check: If the grain cell is not empty when the 920 is turned on, the operator will be prompted to empty the cell and press a key. If this message occurs and there isn't any grain in the cell, then the 920 may require service.

Environmental check: The 920 environmental operating temperature is specified from +22 to +122 °F. If the ambient temperature is outside these limits, a warning message will be displayed.

OTHER SELF-TESTS:

Grain moisture & temperature limits: If the moisture level or temperature of the sample being tested is outside recommended limits a warning message will be displayed.

"Too Low!" or "Too Hi!" Grain moisture too low or too high for selected calibration.

"Temp Lo!" or "Temp Hi!" Grain temperature too low or too high.

Model 920 Moisture Meter Specifications

Environmental operating temperature range: +22 to + 122 deg F

Measurement range: Varies with commodity. Typical moisture ranges are from 6 to 40%

Sample temperature measurement range: +32 to + 120 deg. F (Calibrations with extended sample temperature ranges up to 160 °F are available.)

Sample test time: 5 to 30 seconds depending on sample temperature. Samples that are above 100 deg. or below 40 deg. will take a maximum of 30 seconds to allow for accurate temperature sensing. Samples close in temperature to the meter will take only a few seconds.

Accuracy: The model 920 has been designed to meet or exceed NIST HB44 tolerances for grain moisture meters when used within specified limits.

Dimensions: Width: 5", Depth: 7", Height: 10.5", Weight: 2.7lbs

Display: Large 8-character alphanumeric LCD display with backlight for low-level ambient light conditions.


POWER REQUIREMENTS: The model 920 can be powered from internal batteries, from the supplied external AC adapter, or from an optional automobile lighter adapter. The internal battery pack consists of 6 Alkaline AA batteries. Although the model 920 will operate from standard carbon zinc batteries, alkaline batteries will provide much longer battery life. Alkaline batteries should provide 6 months to a year of intermittent use. Intermittent use is defined as less than 20 tests per week and infrequent usage of the display backlight.

In order to conserve batteries, the model 920 will automatically shift to a low power mode after a few seconds in inactivity, but does not automatically shut off. Always turn off the power switch when the meter is not in use for long periods.

The batteries are automatically bypassed whenever the AC adapter is plugged in. If the model 920 is to be used for an extended period where AC power is available, we suggest operating it from the AC adapter to extend battery life.

REPLACING BATTERIES: To replace the batteries, turn the model 920 upside down and remove the battery cover. Replace the batteries observing correct polarity. If the meter is to be stored for an extended time or the batteries are not required, they should be removed. This will eliminate the possibility of damage from old leaky batteries.

MODEL 920 MOISTURE METER COMPONENTS

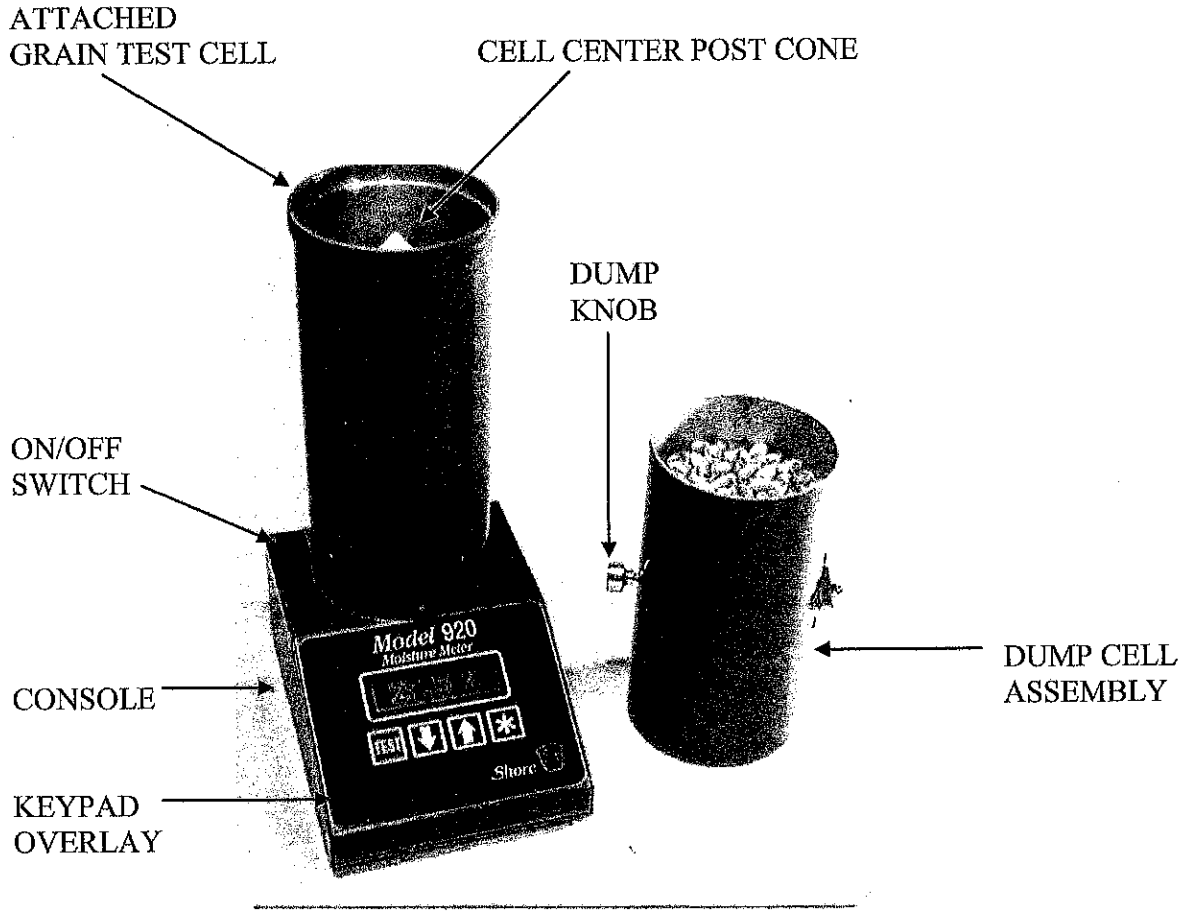

FOR SERVICE, CONTACT

SHORE MEASURING SYSTEMS
105 N. PERRY ST.
ATTICA, IN 47918

Phone (800) 837-0863 (USA only) or (765) 769-3000
Fax (574) 658-8016
Email sales@shoremeasuring.com or visit our website at www.moisturetesters.com